

JC09 Rec'd PCT/PTO 24 JUN 2005

## IN THE UNITED STATES PATENT AND TRADEMARK OFFICE

In re application of :  
Morio NISHIGAKI : **Mail Stop: PCT**  
Serial No. NEW : Attorney Docket No. 2005-1041A  
Filed June 24, 2005 :  
**ULTRASONIC DIAGNOSTIC EQUIPMENT**  
**[Corresponding to PCT/JP2004/011681**  
**Filed August 6, 2004]**

SUBMISSION OF FORMAL REPLACEMENT DRAWINGS

Commissioner for Patents  
P.O. Box 1450  
Alexandria, VA 22313-1450


Sir:

Attached hereto are 5 sheets of formal replacement drawings for Figs. 5b, 6, 7A, 7B and 8 now labeled as "Prior Art".

Respectfully submitted,

Morio NISHIGAKI

By

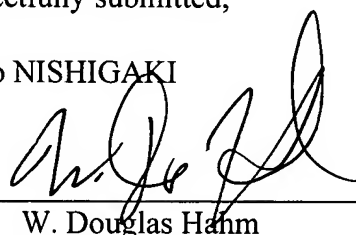

W. Douglas Hamm

Registration No. 44,142

*for*

Nils E. Pedersen

Registration No. 33,145

Attorney for Applicant

THE COMMISSIONER IS AUTHORIZED  
TO CHARGE ANY DEFICIENCY IN THE  
FEES FOR THIS PAPER TO DEPOSIT  
ACCOUNT NO. 23-0975

NEP/WDH/krq  
Washington, D.C. 20006-1021  
Telephone (202) 721-8200  
Facsimile (202) 721-8250  
June 24, 2005

ATTACHMENT G

FIG. 5B PRIOR ART

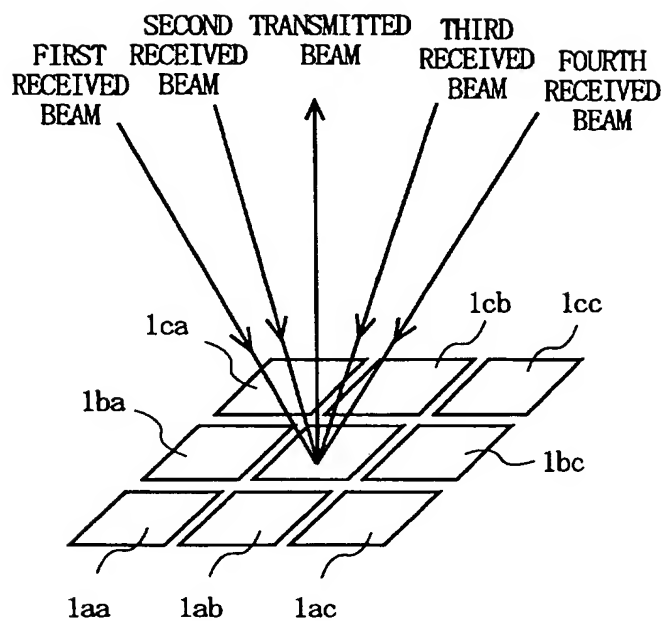


FIG. 6 PRIOR ART

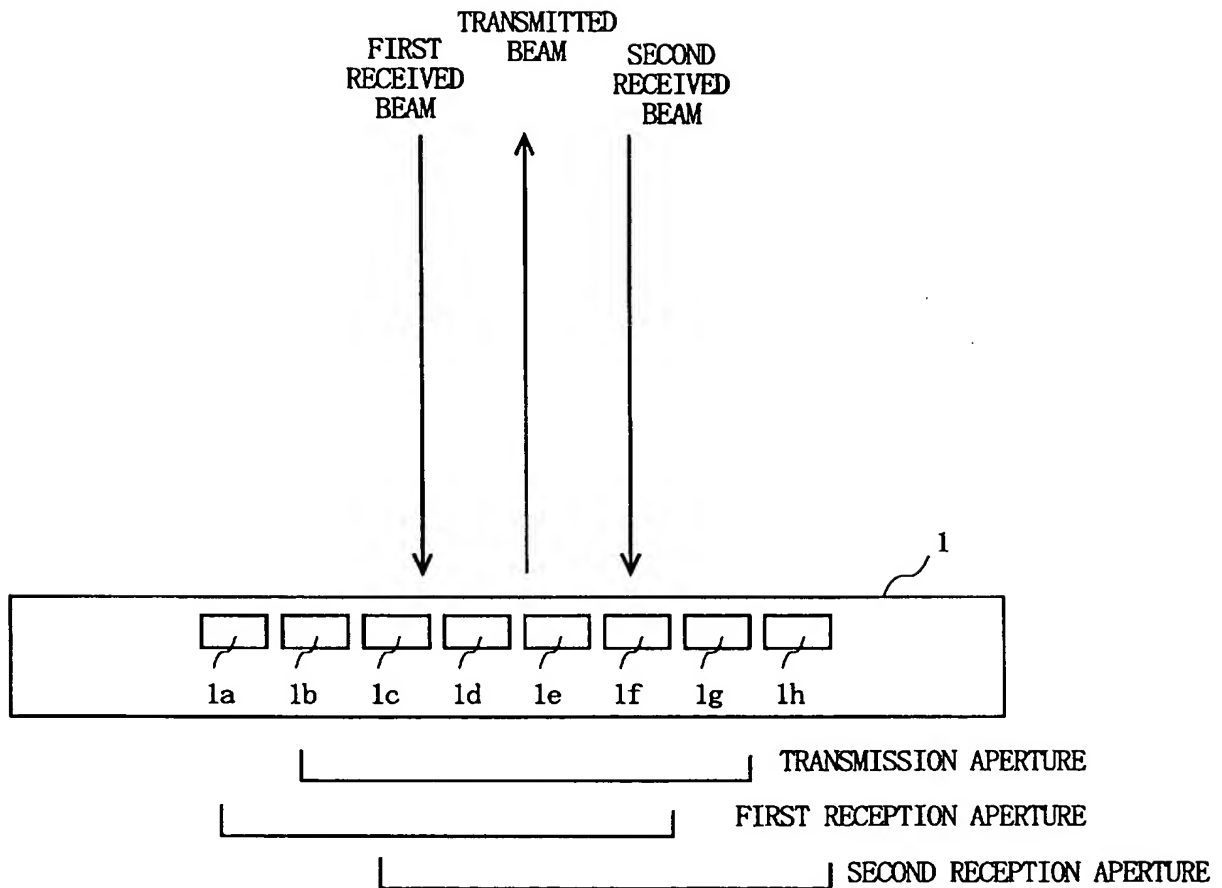


FIG. 7A PRIOR ART

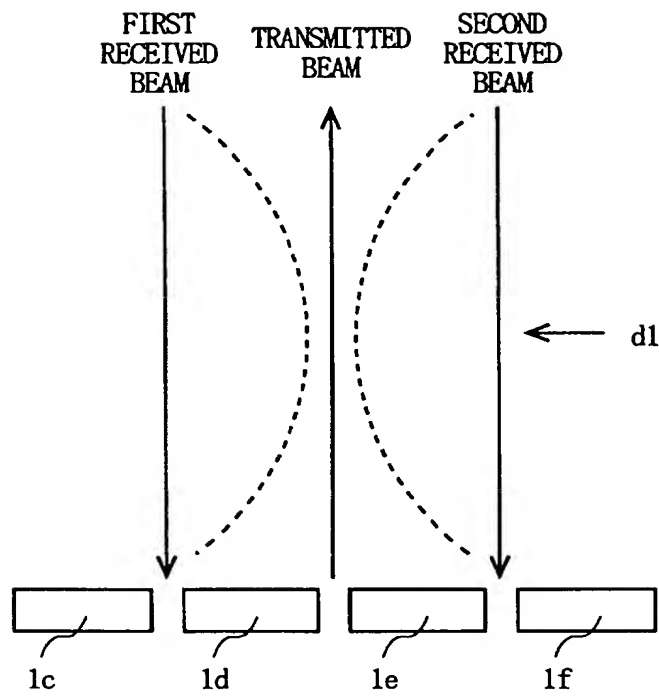


FIG. 7B PRIOR ART

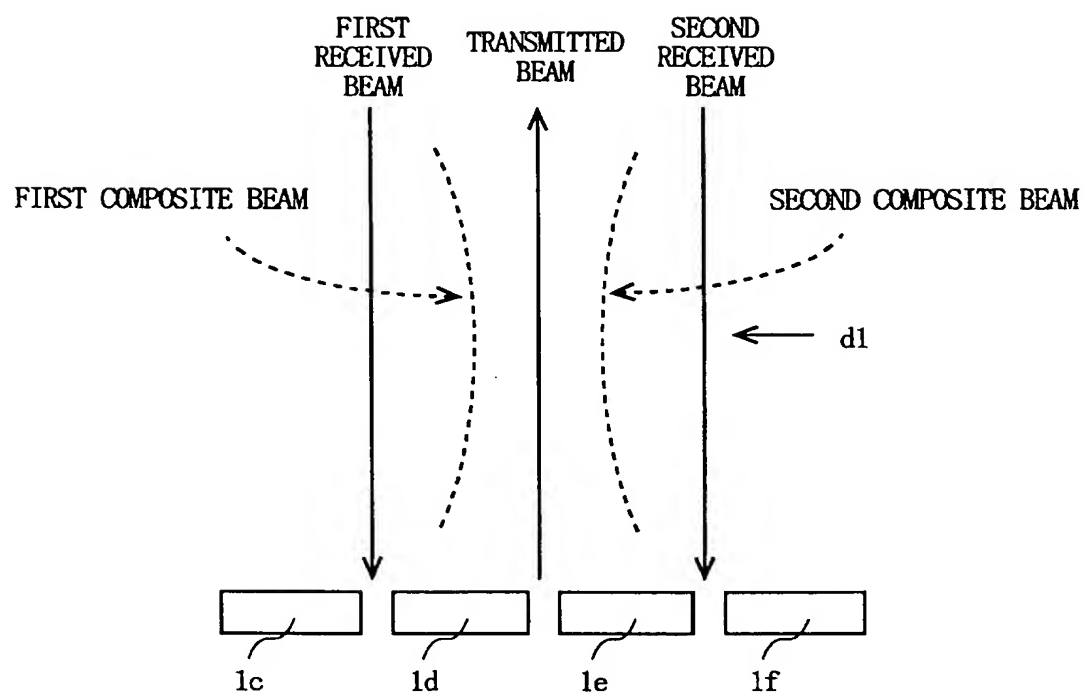


FIG. 8

PRIOR ART

